

Quality Certificate

NC Membrane Filter	Cat Number:MG92345-1PAC
	Lot Number:150710024M

ISO 9001 Quality Standard


The product was manufactured in the Membrane Solutions facility whose Quality Management System is approved by an accredited registering body to the ISO 9001 Quality Systems Standard.

Membrane Filter Lot Characterization

Filter Media	NC	Wettability	Hydrophilic
Color	White	Thickness(μm)	120-150
Pore Size(μm)	0.22	Bubble Point (psi)	61-87
Size(mm)	300*3000	Flow Rate(ml/min/cm ² @10psi)	6.5-12.5

Bubble point and Flow rate are tested by water at 25°C.

HPLC Extractables Test (254nm)

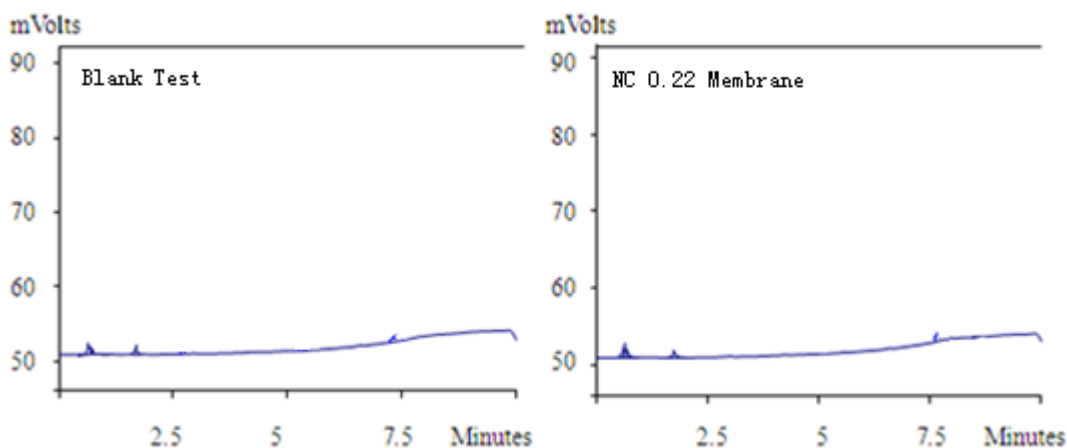

Specification	Result
No detectable peaks	Pass